



These are all test points and miscellaneous passive parts.

These are the linear regulators for the CPLDs (+5V to +3.3V)

These parts are passives for the cryostat control & monitoring block immediately to the right.

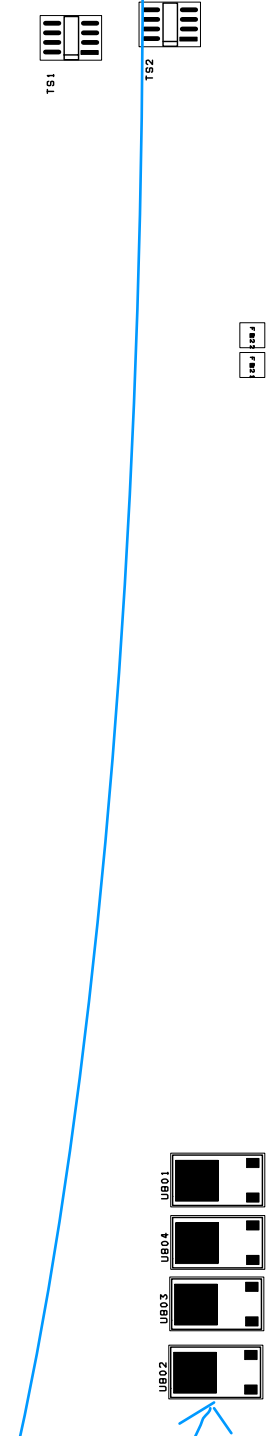

REVISION V1C-FPS

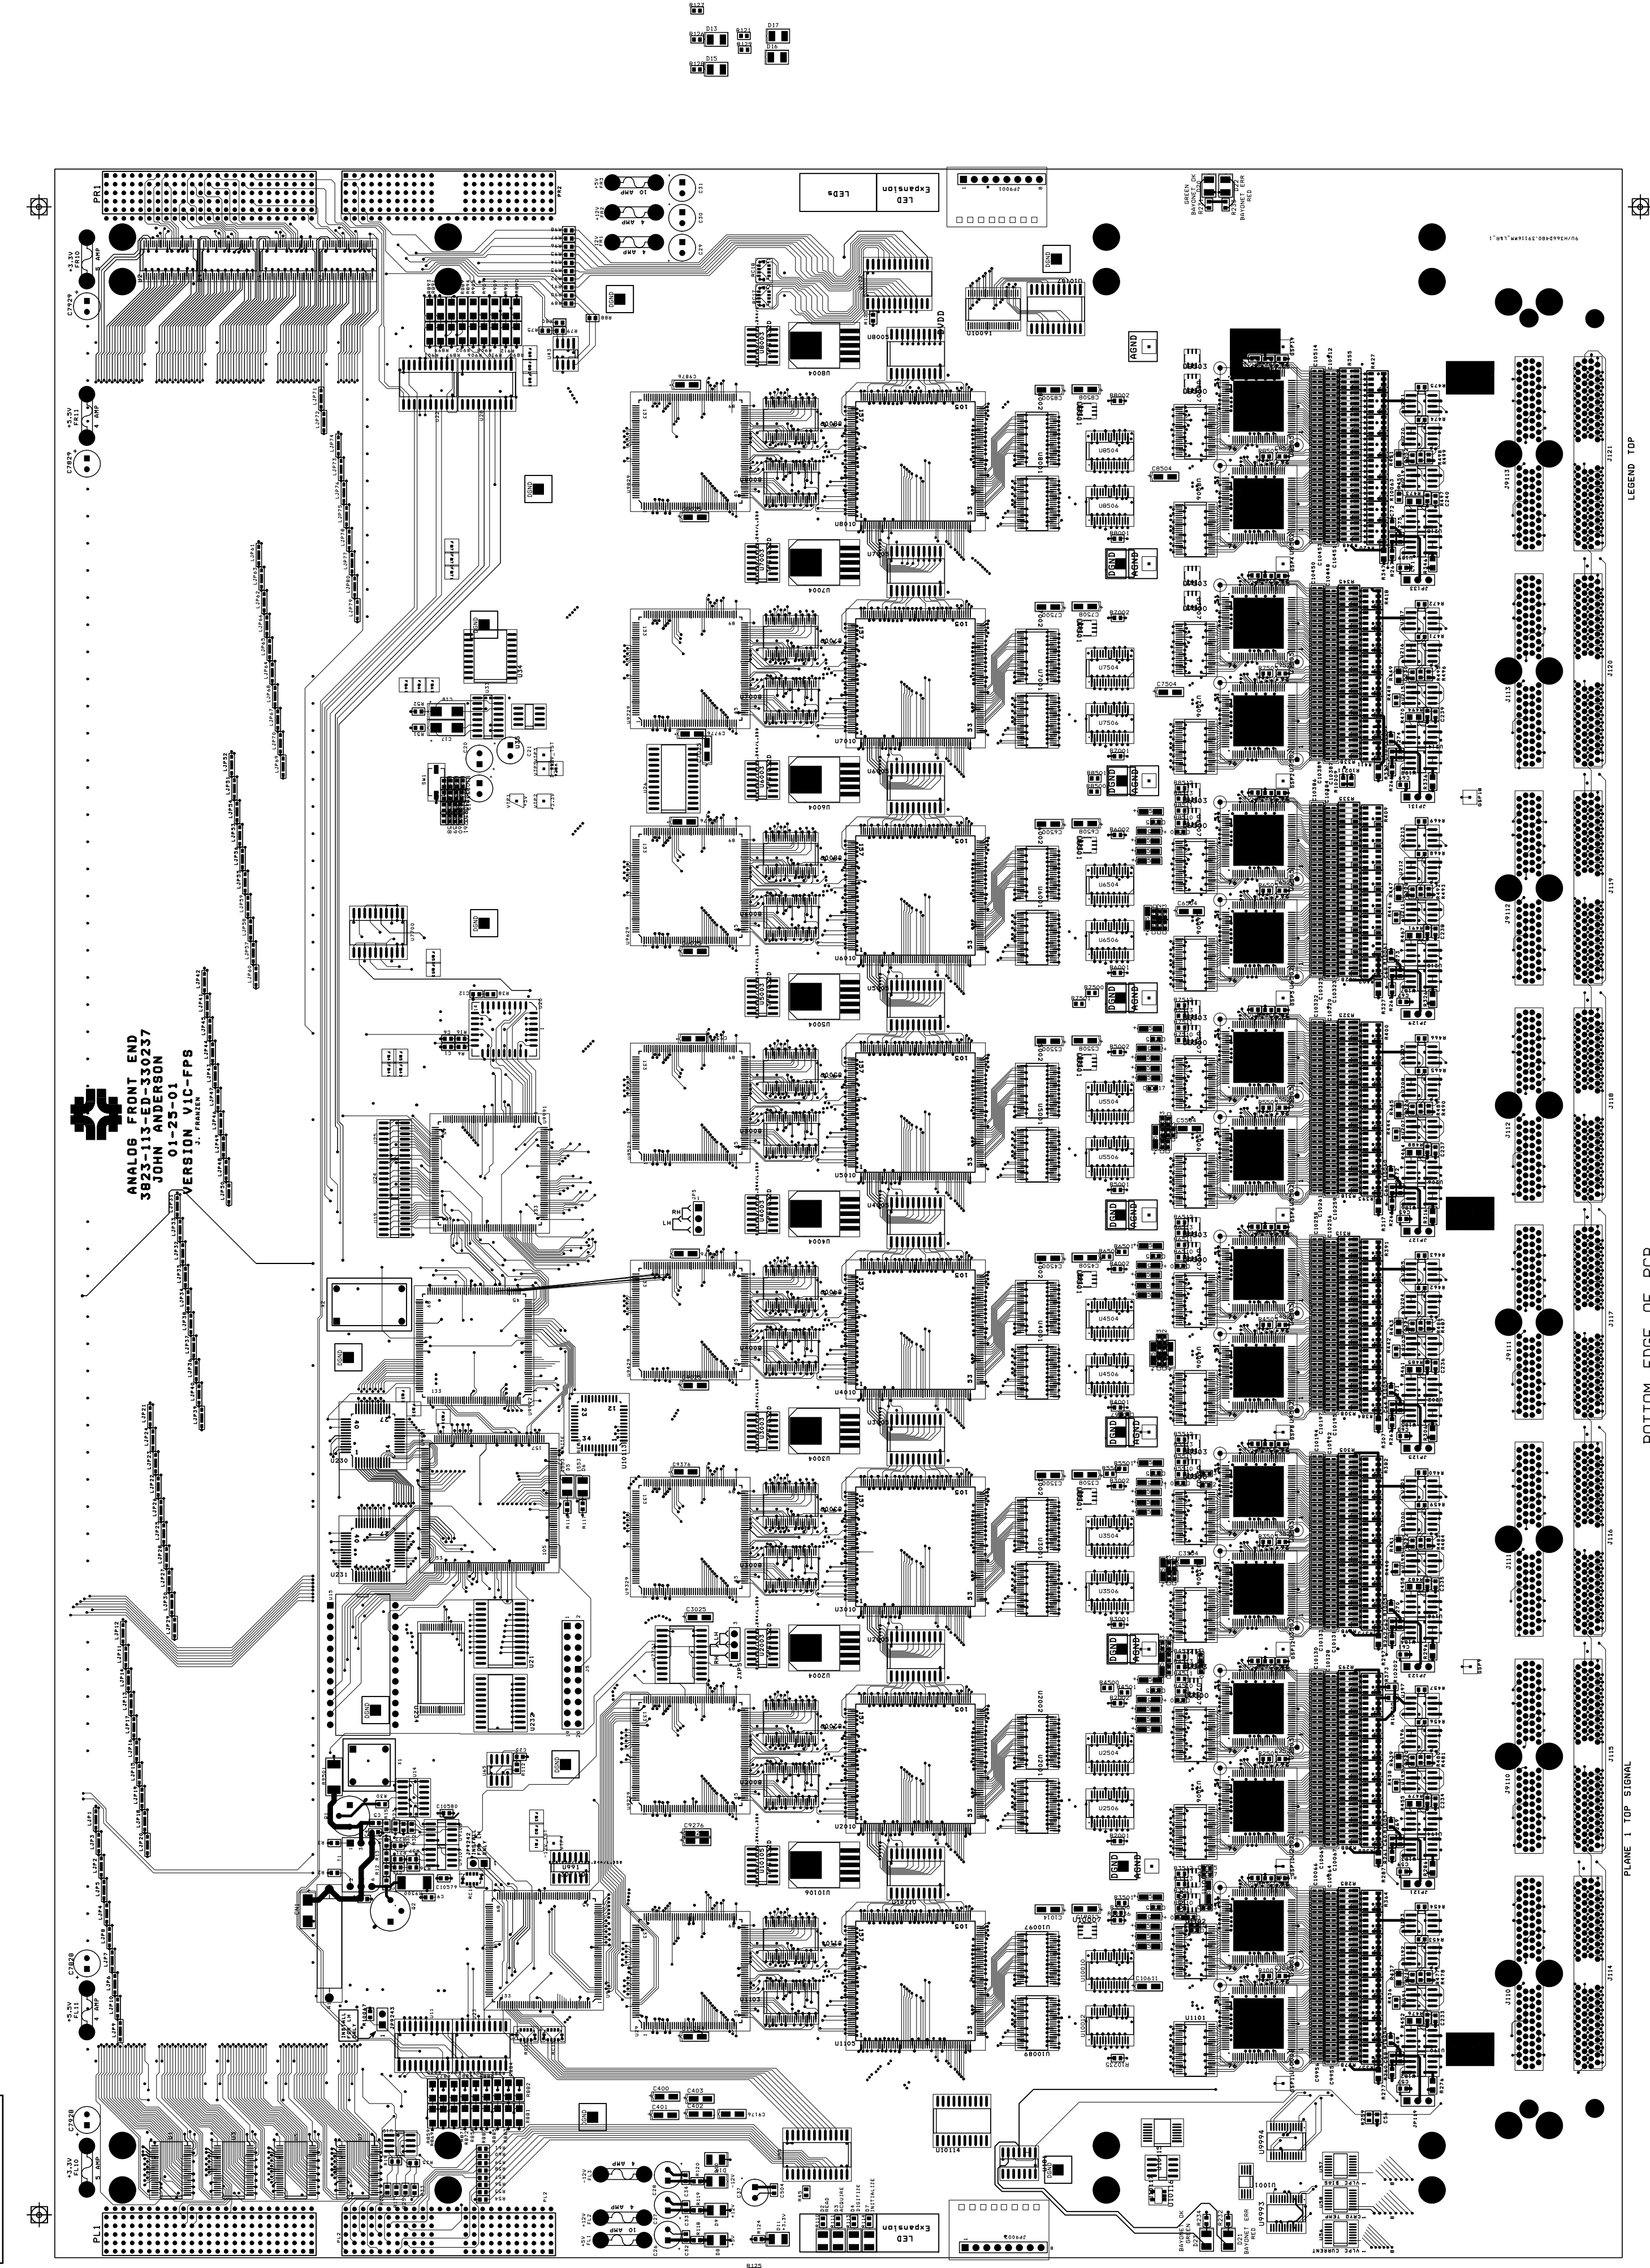

LEGEND TOP

LEADS FOR

